


Software Version : 6.3.1.0504  
Sample Name : BPC-157 - PROBKA NR 3  
Instrument Name : LC-200  
Rack/Vial : 0/0  
Sample Amount : 1,000000  
Cycle : 1

Date : 2021-03-30 15:08:50  
Data Acquisition Time : 2021-03-27 01:35:22  
Channel : A  
Operator : manager  
Dilution Factor : 2,000000

Result File :

Sequence File : C:\PenExe\TcWS\Ver6.3.1\Examples\HPLC- 110-S\ROK 2021\MARZEC\26.03-ald ER\26.03.seq

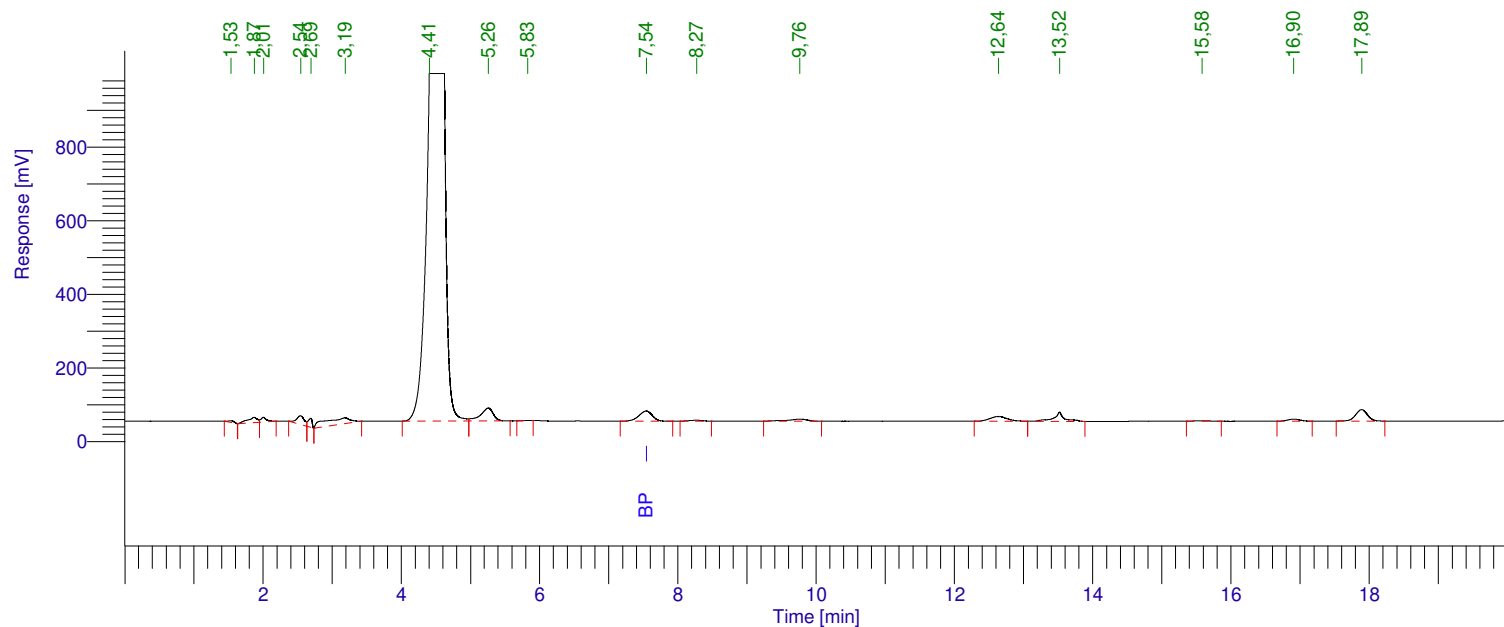

## Raport analizy HPLC

Pik #	Nazwa związku	Czas retencji [min]	Stezenie związku [ug na probka]
10	BPC-157	7,54	232