


Software Version : 6.3.1.0504
Sample Name : BPC-157 - PROBKA NR 6
Instrument Name : LC-200
Rack/Vial : 0/0
Sample Amount : 1,000000
Cycle : 1

Date : 2021-03-30 15:10:02
Data Acquisition Time : 2021-01-27 02:58:47
Channel : A
Operator : manager
Dilution Factor : 2,000000

Result File :

Sequence File : C:\PenExe\TcWS\Ver6.3.1\Examples\HPLC- 110-S\ROK 2021\MARZEC\26.01-ald ER\26.01.seq

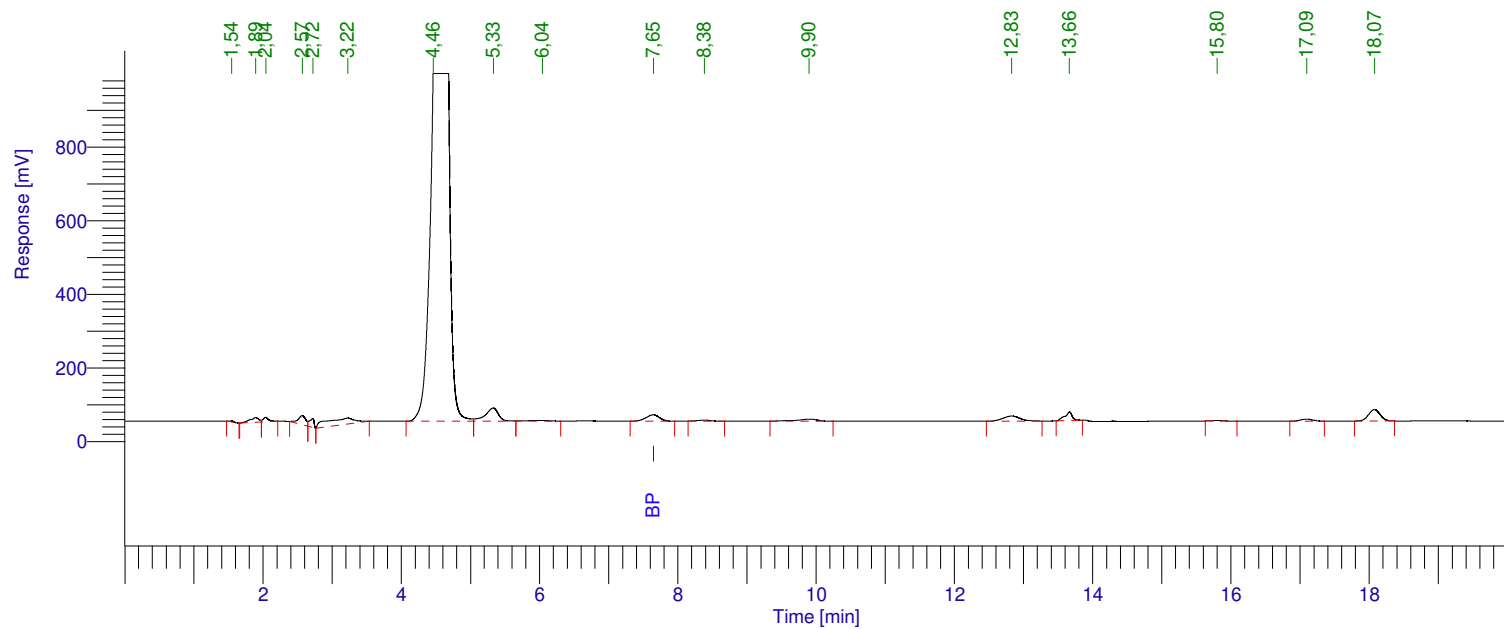

Raport analizy HPLC

Pik #	Nazwa związku	Czas retencji [min]	Stężenie związku [ug na probka]
10	BPC-157	7,65	218