


Software Version : 6.3.1.0504  
 Sample Name : BPC-157 - PROBKA NR 7  
 Instrument Name : LC-200  
 Rack/Vial : 0/0  
 Sample Amount : 1,000000  
 Cycle : 1

Date : 2021-03-30 15:10:23  
 Data Acquisition Time : 2021-013-27 03:26:36  
 Channel : A  
 Operator : manager  
 Dilution Factor : 2,000000

Result File :

Sequence File : C:\PenExe\TcWS\Ver6.3.1\Examples\HPLC- 110-S\ROK 2021\MARZEC\26.03-ald ER\26.03.seq

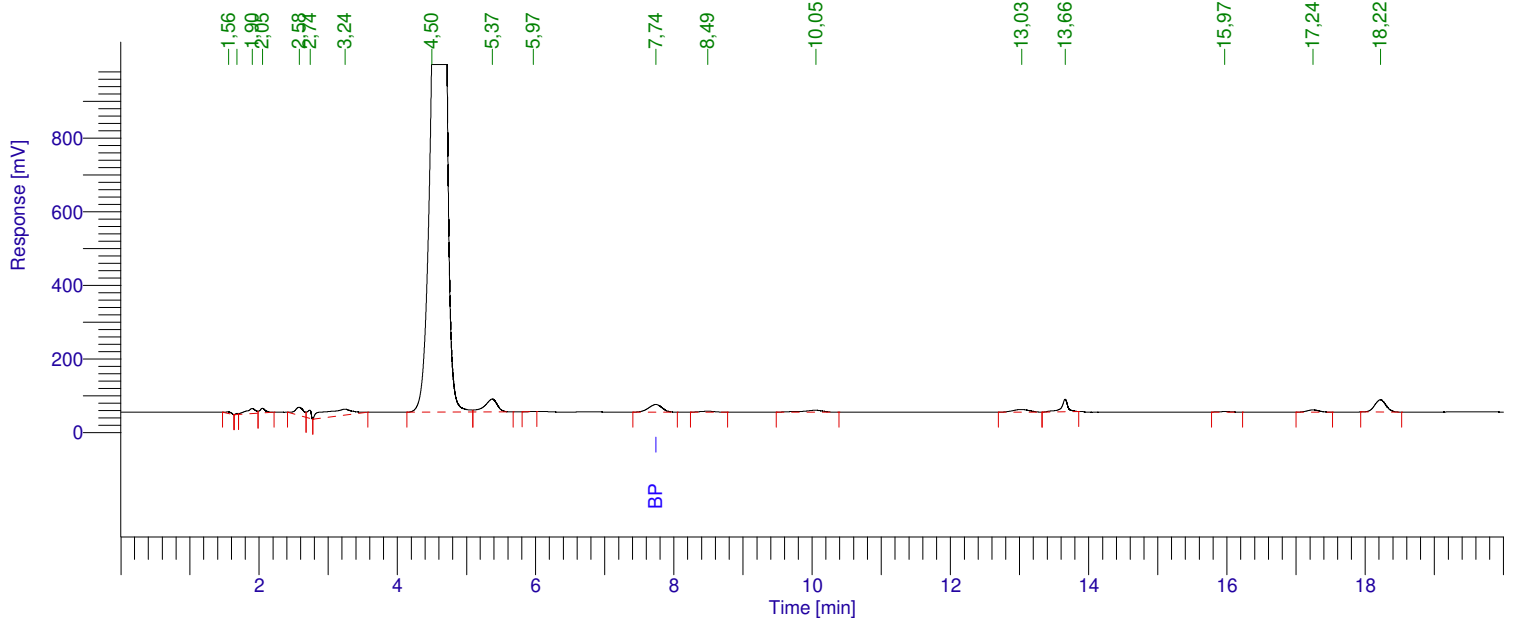

## Raport analizy HPLC

Pik #	Nazwa związku	Czas retencji [min]	Stężenie związku [ug na probka]
11	BPC-157	7,74	224